


HiSpeed CT  
Ex: 11253  
HEAD  
Ser: 202  
Im: 14  
Ax: S85.5

Mag: 1x

DRISCOLL CHILDREN'S HOSPITAL  
JAKAREN GUNTER  
1999 October 5 F 320560  
Acc: 3480264  
2002 June 27  
Acq Tm: 18:07:36

512 x 512  
STANDARD

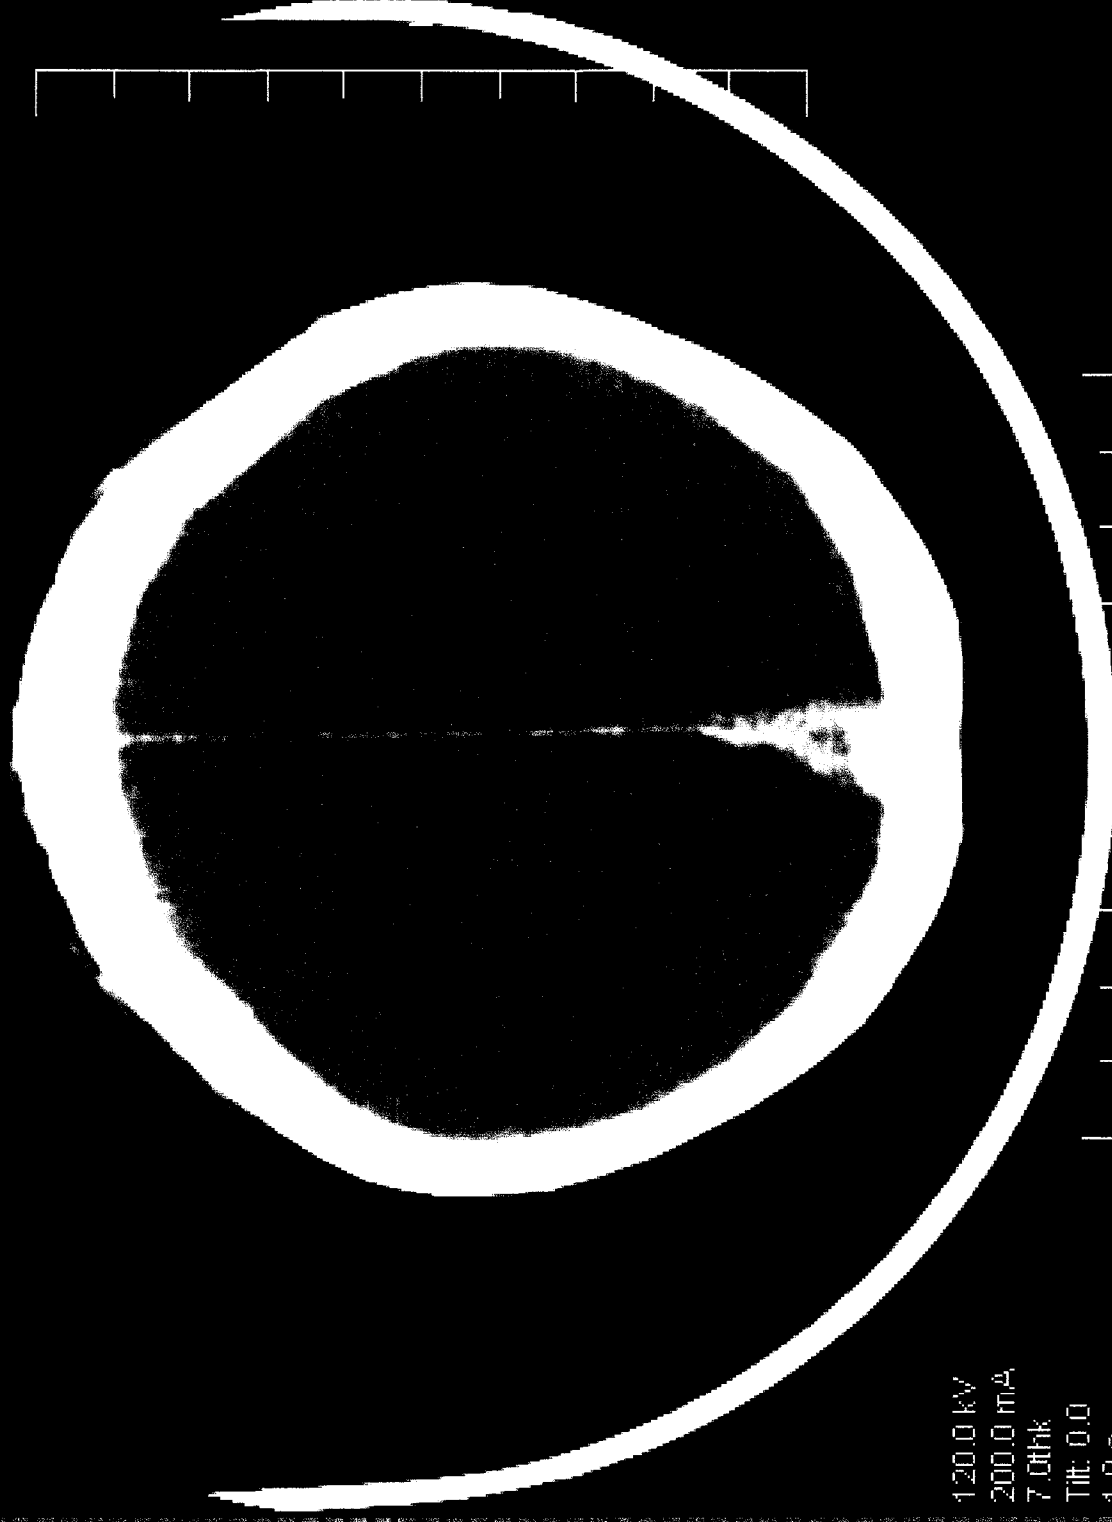

120.0 kV  
200.0 mA  
7.0thk  
Tilt: 0.0  
1.0 s  
WV: 60 L: 40



F

FOV: 20.0 x 20.0cm

DEFENDANT'S  
EXHIBIT  
14